



IRON KIT

OCTA-SLIDE 2, 0.5-10 PPM


CODE 3347-01

QUANTITY	CONTENTS	CODE
30 mL	*Iron Reagent #1	*4450-G
4.5g	*Iron Reagent #2 Powder	*4451-S
4.5g	Ferrous Iron Reagent	4453-S
2	Spoons, 0.05 g, plastic	0696
2	Test Tubes, 2.5-5-10 mL, plastic, w/caps	0106
1	Octa-Slide 2 Viewer	1101
1	Iron Octa-Slide 2 Bar, 0.5 - 10 ppm	4448-01

*WARNING: Reagents marked with an * are considered to be potential health hazards. To view or print a Material Safety Data Sheet (MSDS) for these reagents go to www.lamotte.com. To obtain a printed copy, contact LaMotte by e-mail, phone or fax.

To order individual reagents or test kit components, use the specified code number

USE OF THE OCTA-SLIDE 2 VIEWER

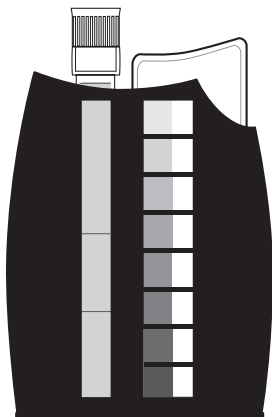










The Octa-Slide 2 Viewer should be held so non-direct light enters through the back of the Viewer. Slide the Octa-Slide 2 Bar into the Viewer. Insert the reacted sample into the top of the Viewer. Match the color of the reaction to the color standards.









WARNING! This set contains chemicals that may be harmful if misused. Read cautions on individual containers carefully. Not to be used by children except under adult supervision

PROCEDURES

TOTAL IRON

<p>1.  Insert Iron Octa-Slide 2 Bar (4448-01) into the Octa-Slide 2 Viewer (1101).</p>	<p>2.  Rinse test tube (0106) with sample water. Fill to 5 mL line.</p>
<p>3.  Add 5 drops of *Iron Reagent #1 (4450).</p>	<p>4.  Cap and mix.</p>
<p>5.  Use the 0.05g spoon (0696) to add one level measure of *Iron Reagent #2 Powder (4451).</p>	<p>6.  Cap and shake until powder dissolves.</p>
<p>7.  Wait 3 minutes.</p>	<p>8.  Insert test tube into Octa-Slide 2 Viewer.</p>
<p>9.  Match sample color to a color standard. Record as ppm Total Iron.</p>	

FERROUS IRON

<p>1.  Insert Iron Octa-Slide 2 Bar (4448-01) into the Octa-Slide 2 Viewer (1101).</p>	<p>2.  Rinse test tube (0106) with sample water. Fill to 5 mL line.</p>
<p>3.  Add 5 drops of *Iron Reagent #1 (4450).</p>	<p>4.  Cap and mix.</p>
<p>5.  Use the 0.05g spoon (0696) to add one level measure of Ferrous Iron Reagent (4453).</p>	<p>6.  Cap and shake until powder dissolves.</p>
<p>7.  Insert test tube into Octa-Slide 2 Viewer.</p>	<p>8.  Match sample color to a color standard. Record as ppm Ferrous Iron.</p>
<p>To calculate ppm Ferric Iron: Ferric Iron = Total Iron - Ferrous Iron</p>	

LaMOTTE COMPANY

Helping People Solve Analytical Challenges®

PO Box 329 • Chestertown • Maryland • 21620 • USA
800-344-3100 • 410-778-3100 (Outside U.S.A.) • Fax 410-778-6394

Visit us on the web at www.lamotte.com